

MedPark

S1

**NEW BONE
NEW LIFE**

DENTAL
NATURAL BONE SUBSTITUTE

CE
1434

Concept of customized Bonegraft material




Sticky Bone without Blood Collection!

Bovine Bone Mineral



- Unable to mold
Lack of retentivity
- Scattered & Flowing
- Blood collection to make sticky bone



- Moldable & Customizing
- Customized build up
- Sticky bone made easily with saline or blood

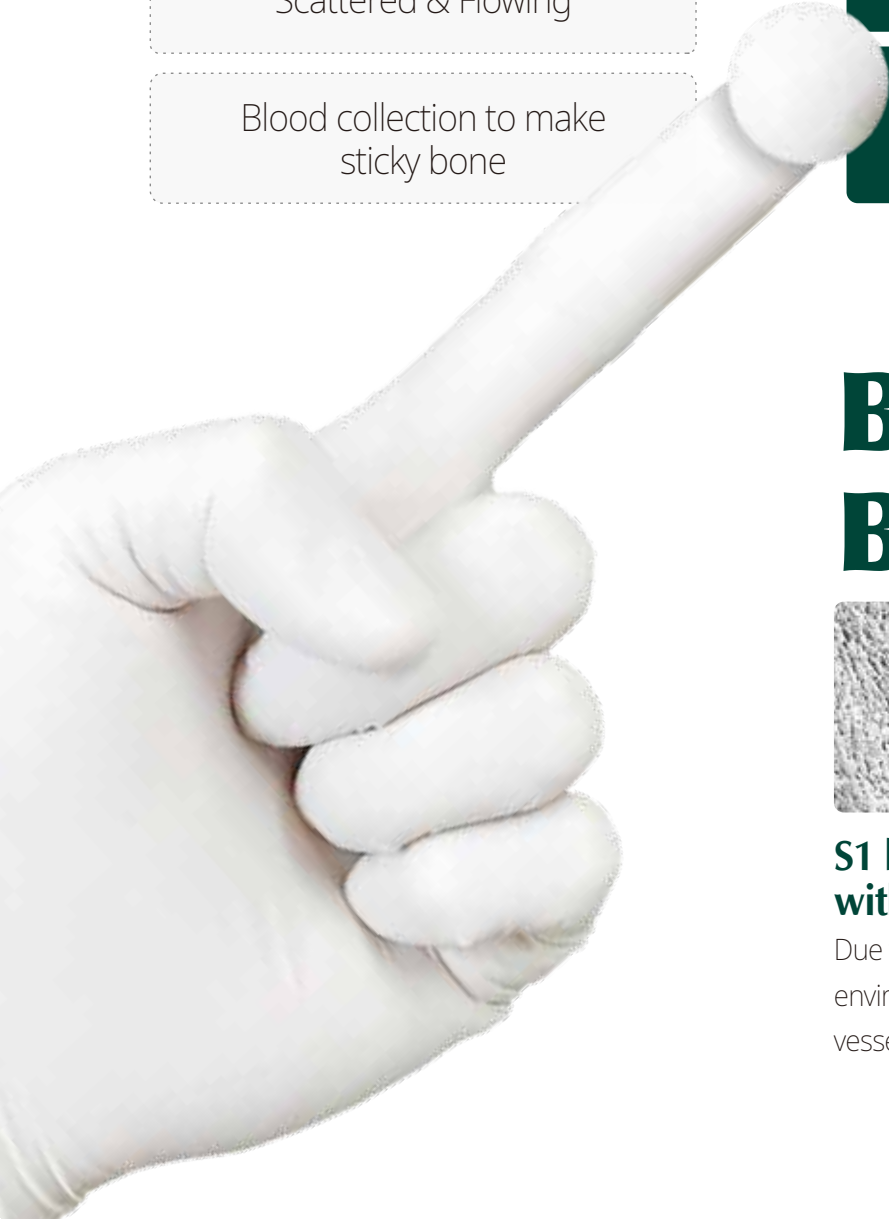

BOVINE BONEGRAFT

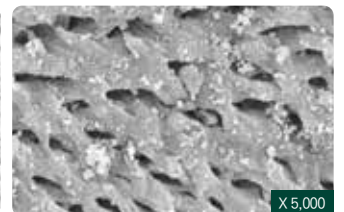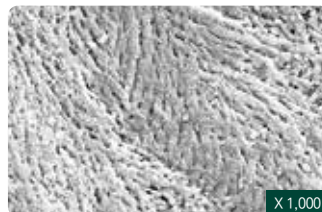

S1 has similar structural characteristics with human bones

Due to its high porosity, S1 provides the most optimal environment for promoting osteoblast adhesion, blood vessel formation, and bone regeneration.

NEW BONE NEW LIFE

Keywords



S1 (Bovine Bone)



Bovine Bone Mineral


- 1 Excellent adhesion and fixation
- 1 Rigid Space Maintenance
- 1 Excellent osteoconduction



S1 (Bovine Bone)

- 1 Easy to manipulate
- 1 Various indications

1 High porosity



Porosimeter Test

- Percentage of porosity is more than 70%
- High porosity allows rapid penetration of growth factors

1 Improved Hydrophilicity



Hydrophilicity Test

- Porous structure makes blood circulation easily


1 Excellent shape maintenance



Pressure Test

- Perfect shape maintenance against high pressure from outside compared to other bone

1 Bone formation rate

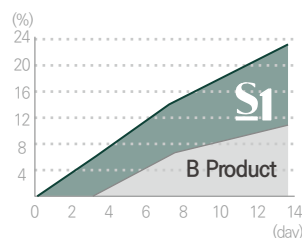

Mass Increase Test

- High attachment rate of ions to S1
- 21% increase in mass after 14days due to high adhesive rate of ions


Quick Guide

Please apply the liquid as indicated


Each package is for one-time use only

Do not mix with other bonegraft


Mix with solutions well enough

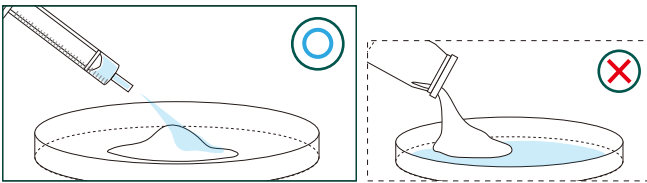


1 Place S1 in the tray and hydrate the materials with saline

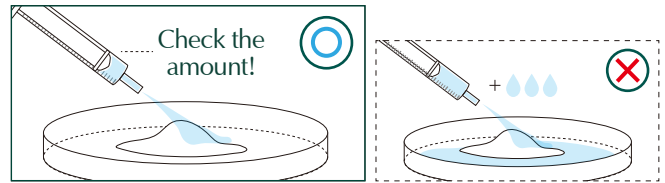

1 Please use the recommended amount of saline only.

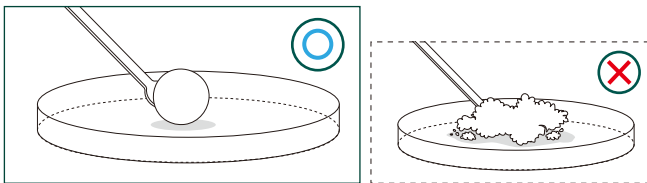

1 Knead the dough enough for at least 30 seconds by using hands or tools to form a lumpy shape before using S1.

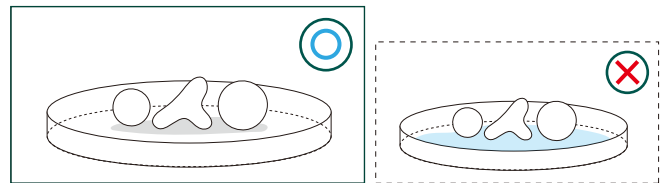

1 Do not soak in saline after shaping for a surgery

Recommended Amount of Saline

TYPE	PARTICLE SIZE	WEIGHT	SOLUTION AMOUNT
Powder	0.2~1.0 mm	0.15 g	0.2 cc
		0.25 g	0.35 cc
		0.5 g	0.7 cc
		1.0 g	1.4 cc
		2.0 g	2.8 cc

TYPE	PARTICLE SIZE	WEIGHT	SOLUTION AMOUNT
Chip	1.0~2.0 mm	0.25 g	0.45 cc
		0.5 g	0.9 cc
		1.0 g	1.8 cc
		2.0 g	3.6 cc

* Ordermade : Medium Type (0.5~1.4 mm)

Innovative technology

Check it out for yourself !



Watch the clinical uses on our Youtube



Biopsy

※ Hematoxylin & Eosin Stain

Case 1 | #14, Ridge augmentation

Patient Info : 65 years-old, female

Clinical Opinion

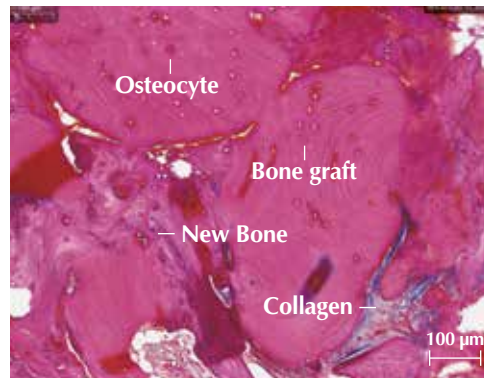
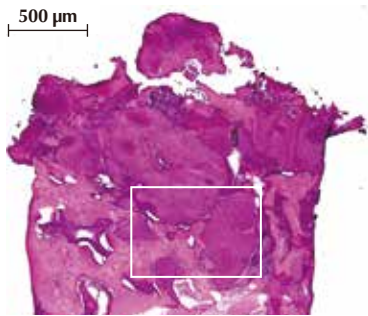


- Excellent bone formation around bone graft material
- The graft materials appeared surrounded by newly formed bone
- No sign of inflammation or immune rejections

Case 2 | #26, Sinus graft

Patient Info : 73 years-old, female

Clinical Opinion

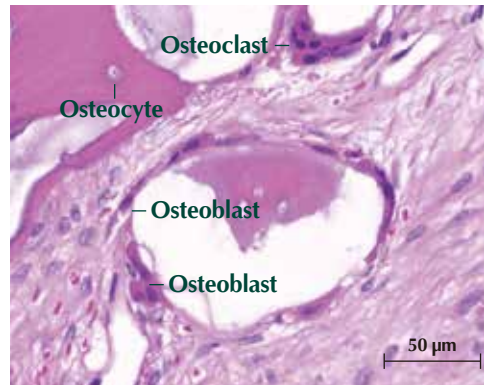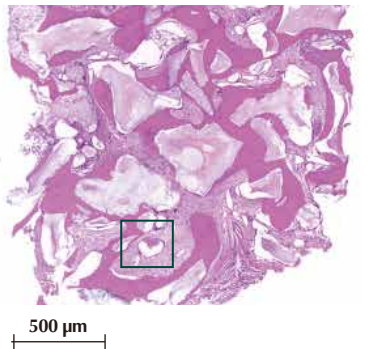

- Excellent osteoconduction as it shows osteoclasts and new bone formation
- No evidence of inflammation or immune rejection

Clinical cases

Case 1

Patient Info : 59 years-old, female, Ridge augmentation



Before surgery




Placing Fixture




Grafting S1



Suture



After grafting S1



Final prosthesis

Case 2

Patient Info : 66 years-old, Male, Ridge augmentation



Before surgery



Dehiscence defect and widespread bone defects



Grafting S1



4 months after grafting S1



Postoperative x-ray, after 4 month



Final prosthesis

MedPark



E-mail biz@medpark.net
www.medpark.net